

## 1 Introduction

*E-Guide* is a light-curing material for the additive manufacturing of individual dental surgical drill guides. *E-Guide* has been optimized for use with Desktop Health's *Einstein* and *Einstein Pro XL* and EnvisionTEC's *Perfactory® DDP (Digital Dental Printer) series, Perfactory® Vida and Perfactory® Vida cDLM, Perfactory® MicroPlusXL, Perfactory EnvisionOne cDLM, Perfactory® P4K series and Perfactory® D4K* machines and may only be used with these machines and the corresponding software systems. *E-Guide* is a medical device classified as class 1 according to 21 CFR part 872 and classified in Canada as Class 1 according to Medical Device Regulations (SOR/98-282). Surgical drill guides from *E-Guides* may only be manufactured by dental technicians and used on a patient by authorized users such as dentists or oral surgeons.

The following Instruction for Use includes safety and environmental information and the instructions for the manufacturing and post-processing procedures of the product, which must be strictly adhered to.

## 2 Indication

*E-Guide* is intended for the additive manufacturing of individual dental surgical drill guides, which serve as guiding aids for navigated-/ 3D-implantology of dental implants. These are intended as a precautionary protective measure to prevent injuries to nerves, blood vessels and jawbone. Surgical drill guides are used by dentists or oral surgeon prior to the surgical procedure in order to allow an exact drilling and thereby an exact placement of the dental implants in the patient's jawbone .

Surgical drill guides from *E-Guide* are custom-made products for single use during the surgical procedure, under consideration of their application and intended exclusively for one patient.

The target group are patients with missing teeth, whereby high-risk patients are excluded.

The minimum approved wall thickness is 3mm and the maximum approved wall thickness is 10 mm. Surgical drill guides can be printed horizontally and vertically orientated. The horizontally (0° in relation to the build platform) orientated dental bite splints need to be supported from outer surface, which is in contact to the opposite jaw. The vertically (90° in relation to the build platform) orientated dental bite splints need to be supported from labial/ vestibular surface. After several printing processes the product may show slight color changes. However, this does not reduce the quality of the application.

## 3 Contraindication

*E-Guide* may only be used for the production of dental surgical drill guides. Any deviation from the Instruction for Use can negatively affect the chemical and physical properties. Consequently, the biocompatibility of the surgical drill guides cannot be guaranteed. *E-Guide* may not be used for the production of x-ray guides.

For patient and users:

Patients, users or third parties who come in contact with products from *E-Guide* must be informed about any side effects before use. *E-Guide* products may not be used if there are known allergies to any of the ingredients, otherwise possible side effects such as shortness of breath, gastrointestinal complaints, dizziness, anaphylactic reactions or shocks, itching and tearing (watery) eyes, headaches or reactions of the skin or mucous membrane such as irritation, rash, swelling, inflammation, redness, wheals or blisters or other allergic reactions may occur.

## 4 Composition

Acrylate/Methylacrylates, methacrylated Oligomers and Monomers, photo initiators, colorants/dyes and absorbers

## 5 Warning

Do not substitute any of the components of the device system, i.e., device resin materials, scanners, printers, post-curing units, CAD/CAM software, templates and tools. Use only those specifically identified in this labelling. Contact the manufacturer for compatible components.

## 6 Hazard and Precaution statements

### Warning:

Causes skin irritation.

May cause an allergic reaction.

Causes serious eye irritation.

Suspected of damaging fertility.

Wear protective gloves, protective clothing, eyes protection, face protection.

### First Aid:

If on skin wash with plenty of water.

If in eyes rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do.

Continue rinsing.

If swallowed, immediately call poison center.

## 7 Storage conditions and und expiry date

The resin needs to be stored in the original packaging between 41 86°F. While removing the resin it must be protected from exposure to light, as spontaneous polymerization is possible. The bottle must be tightly closed after every usage and material removal. Resin inside the machine tray can be re-used for several build jobs. If the level in the tray is too low for subsequent jobs, resin from the bottle can be added as necessary. If the material is not in use, it must be filled back into the bottle. For further information on re-using and mixing material, please check the machine manual. An expiration date is given on the label of every product bottle. The use of expired material is not permitted. The surgical drill guides need to be protected from exposure to light before the final use and during the not usage and storage.

## 8 Notes on disposal

Dispose of contents and container in accordance with local regulation.

The manufactured surgical drill guides, which are used on patients are surgical devices and must be disposed properly due to the risk of infection (contaminated by substances of human origin).

## 9 Instruction disinfection and sterilization

If necessary, the surgical drill guide made of *E-Guide* can be disinfected before use with the following disinfectants: Cidex OPA or a 70 % Ethanol-solution. The disinfecting solutions must be used according to the manufacturer instructions.

Surgical drill guides from *E-Guide* cannot be sterilized.











## 10 Use of software systems and products from other manufacturer

The use of certified software systems for generating the STL-data and the use of sleeves for surgical drill guides and their additional products depends on user's assessments.


## 11 Delivery unit, symbol explanation and manufacturer information

Delivery unit: E-Guide is available in containers of 1 kg

### Symbol explanation:


 <b>LOT</b>	Batch number		Protect from sunlight
	Expiration date		Follow Instruction for Use
	Manufacturer		Temperature limit
 <b>REF</b>	Purchase order number		Production date
 <b>Rx Only</b>	Prescription device labeling statement	 <b>UDI</b>	Unique device identification

## 12 Manufacturing process

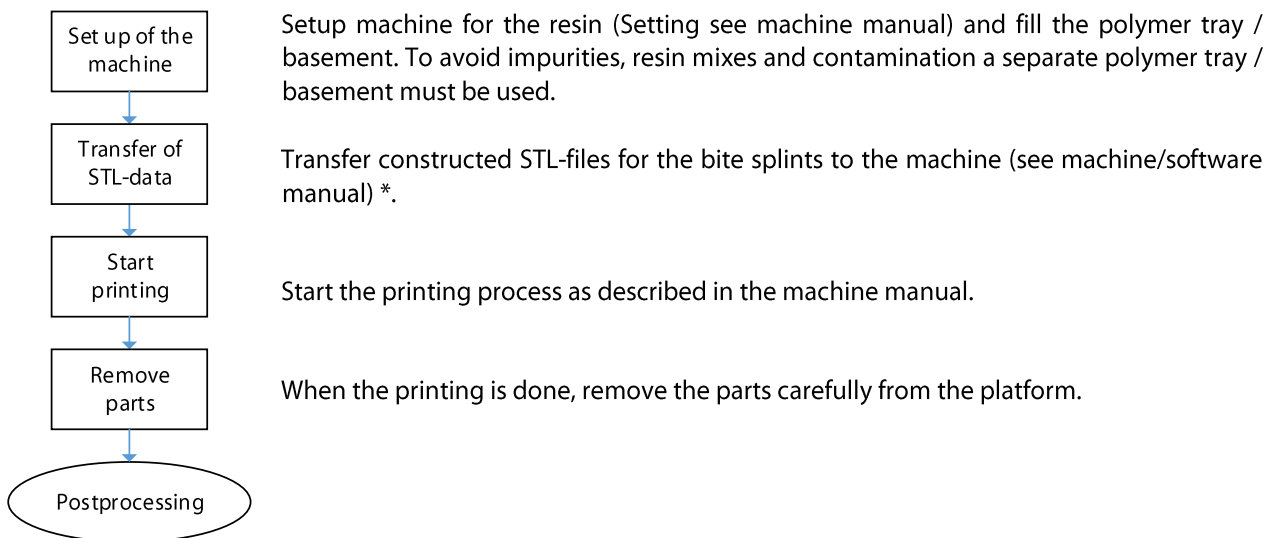

\*The scanning and construction of patients STL data is the responsibility of the customer. We recommend that only trained dental personnel perform the scanning and design. Further, a certified software such as, e.g. 3Shape is recommended. To generate the support structures, we recommend the Perfactory® RP Software (version 3.1540.1602 or later), EnvisionOne RP (version 1.0.1165 or later) or the Cambridge Software from 3Shape (version 2015 2650 or later).

## 13 Postprocessing

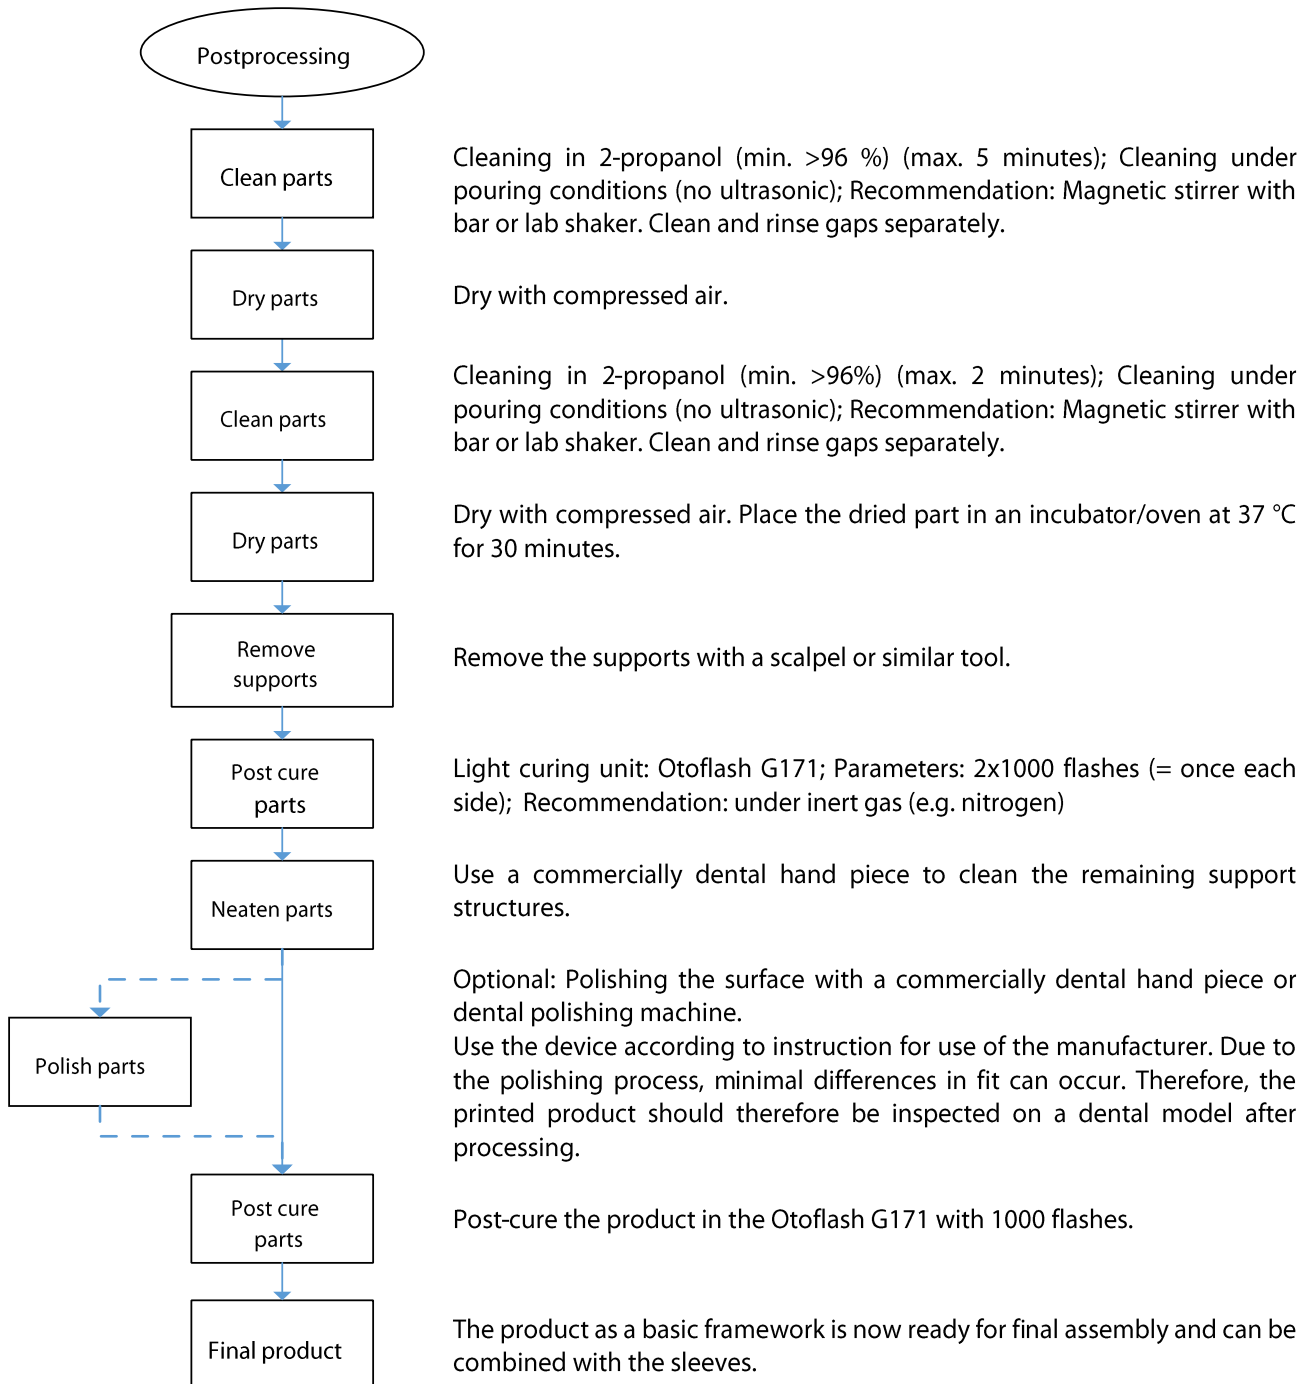

Finally, the completed drill guide can be used on the patient.

Maintain and calibrate equipment according to manufacturer instructions. Using an alternative light source can affect the properties of the final product. It is not allowed to do manual correction by material removal.

## 14 Reporting undesirable effects

In the event of adverse effects, reactions or similar occurrences arising from the use of this products, including those not listed in this Instruction for Use, these must be reported immediately by opening a support ticket via our website <https://envisiontec.com/> or by contacting your local distributor.

## 15 Manufacturer

### EnvisionTEC GmbH

Brüsseler Str. 51                      Phone: +49-(0)2043-98750  
45968 Gladbeck                      E-Mail: info@envisiontec.com  
Germany                                Website: www.envisiontec.com

Revision 08, 17.04.2023